




## Certificate of Analysis

### SALSA® MLPA® Probemix P038 CLL-2

<b>Catalogue #</b>	<b>P038-025R, P038-050R, P038-100R</b>	
<b>Product name</b>	<b>Probemix P038 CLL-2</b>	
<b>LOT</b>	<b>B1-0822</b>	
	25, 50, or 100 reactions.	
Shipping conditions	Dry ice or cooling elements.	
	Store upon arrival between -25°C and -15°C.	
	Expiration date: August 2027, when stored at recommended conditions. This product should not be frozen/thawed more than 25 times.	
Purpose	This product has been developed to determine the DNA copy number of several chromosomal regions and genes such as: 10q23 ( <i>PTEN</i> ), 11q ( <i>ATM</i> ), chromosome 12, 13q14 ( <i>RB1</i> , <i>DLEU1/2</i> ), 14q, 17p13 ( <i>TP53</i> ) and chromosome 19. This probemix can also be used to detect the presence of <i>NOTCH1</i> p.P2514Rfs*4, <i>SF3B1</i> p.K700E and <i>MYD88</i> p.L265P point mutations. This probemix is designed for use only in combination with SALSA MLPA reagent kits, SD029 and Coffalyser.Net analysis software as described in the MLPA General Protocol.	
Quality control specifications	<ul style="list-style-type: none"> <li>- Sufficient distance between peaks, absence of extra or shoulder peaks, and completeness of hybridisation of each individual probe, as tested on Applied Biosystems and Beckman/SCIEX GeXP sequencers.</li> <li>- Standard deviation of each individual probe <math>\leq 0.10</math>, when tested on 23 different DNA samples of healthy individuals, extracted by various methods.</li> <li>- Each individual probe meets reaction-specific criteria when tested on a single DNA sample under various experimental conditions.</li> <li>- No-DNA controls result in only five major peaks shorter than 121 nucleotides (nt): four Q-fragments at 64, 70, 76 and 82 nt, and one peak in the range of 0-40 nt corresponding to the unused portion of the fluorescent PCR primer. Non-specific peaks longer than 121 nt AND with a height &lt;25% of the median of the four Q-fragments are not expected to affect MLPA reactions when sufficient (50-250 ng) sample DNA is used. Note: We observed two prominent peaks above the 25% threshold with lengths of approximately 147 nt and 349 nt in a No-DNA control in case the ligation reaction was performed at room temperature.</li> </ul>	Test result
		PASS


None of the ingredients are derived from humans, animals, or pathogenic bacteria. Based on the concentrations present, none of the ingredients are hazardous as defined by the Hazard Communication Standard. **A Safety Data Sheet (SDS) is not required for these products:** none of the preparations contain dangerous substances (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and amendments) at concentrations requiring distribution of an SDS (as per Regulation (EC) No 1272/2008 [EU-GHS/CLP] and 1907/2006 [REACH] and amendments). If spills occur, clean with water and follow appropriate site procedures.

<b>More information:</b> <a href="http://www.mrcholland.com">www.mrcholland.com</a> ; <a href="http://www.mrcholland.eu">www.mrcholland.eu</a>	
	MRC Holland bv; Willem Schoutenstraat 1 1057 DL, Amsterdam, The Netherlands


E-mail	<a href="mailto:info@mrcholland.com">info@mrcholland.com</a> (information & technical questions) <a href="mailto:order@mrcholland.com">order@mrcholland.com</a> (orders)
Phone	+31 888 657 200

## Certificate of Analysis

### SALSA MLPA Probemix P038 CLL-2 sample picture

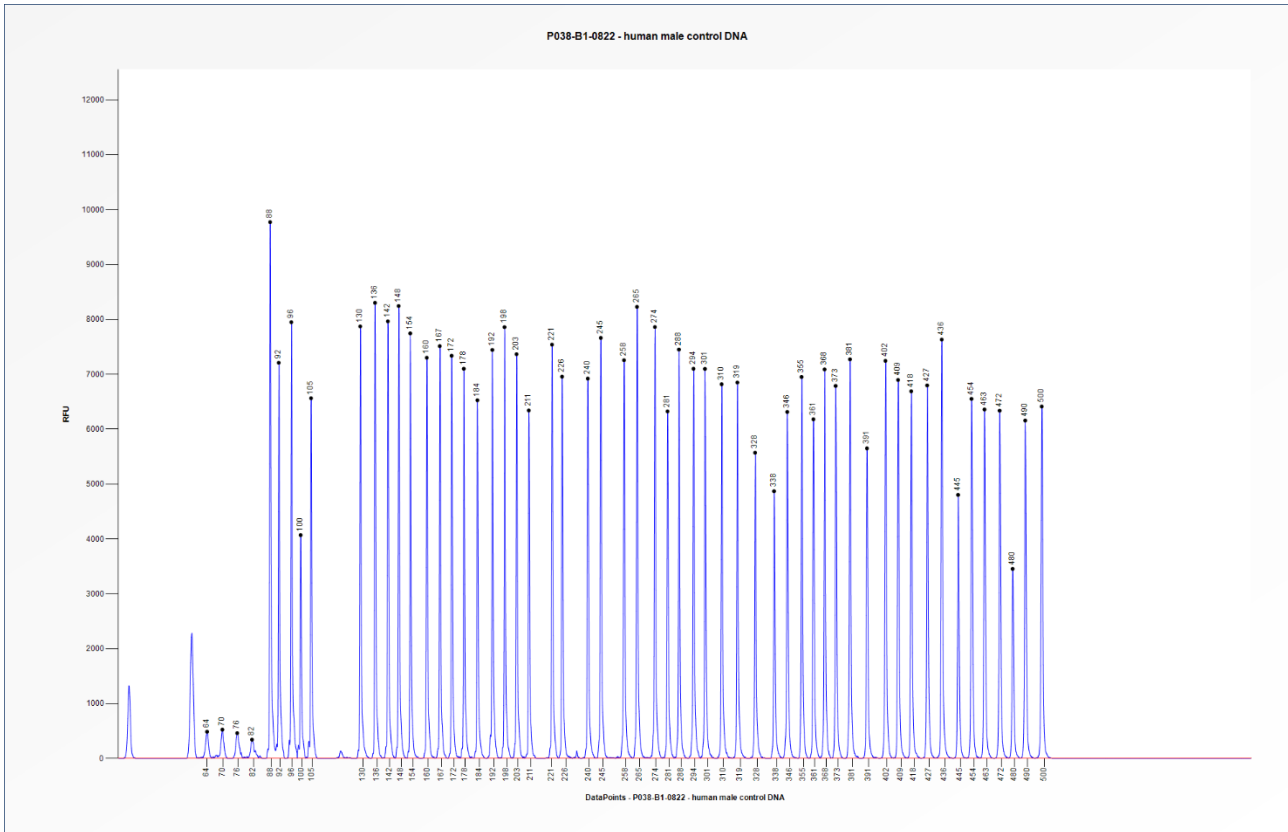

**Figure 1.** Capillary electrophoresis pattern from a sample of approximately 50 ng human male control DNA analysed with SALSA MLPA Probemix P038 CLL-2 (B1-0822).

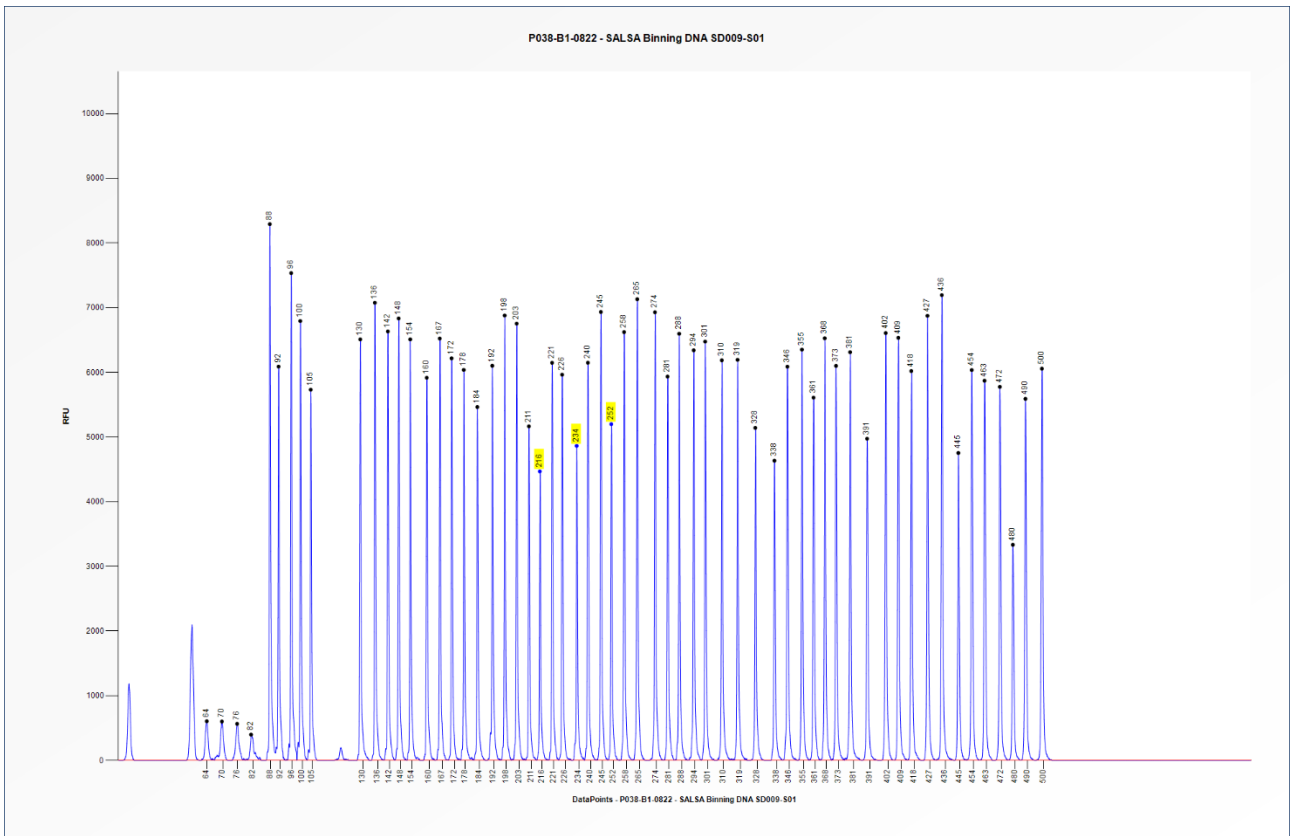

**Figure 2.** Capillary electrophoresis pattern from SALSA Binning DNA SD009-S01 (approximately 50 ng) analysed with SALSA MLPA Probemix P038 CLL-2 (B1-0822). The locations of the *NOTCH1* p.P2514Rfs\*4, *SF3B1* p.K700E and *MYD88* p.L265P mutation-specific probes at 216 nt, 234 nt and 252 nt, respectively, are indicated.

**This lot was certified by MRC Holland on 12 April 2023.**

This certificate is a declaration of analysis at the time of the manufacturing process. All assays were run in compliance with manufacturer’s instructions for use.

Implemented changes in the COA
Version 01 – 12 April 2023 (6) - Not applicable, new document.